

PE15-030

FLAT CHRYSLER

11-24-2015

ENCLOSURE 4


CAIR Backup


25109804





USE 8-SPECS
ONLY USE DIAGNOSTIC TOOL TO DETERMINE
FLUID 68157995AA
LEVEL AT TEMP 86-122°F/30-50°C
PRESSURE MUST OPEN!

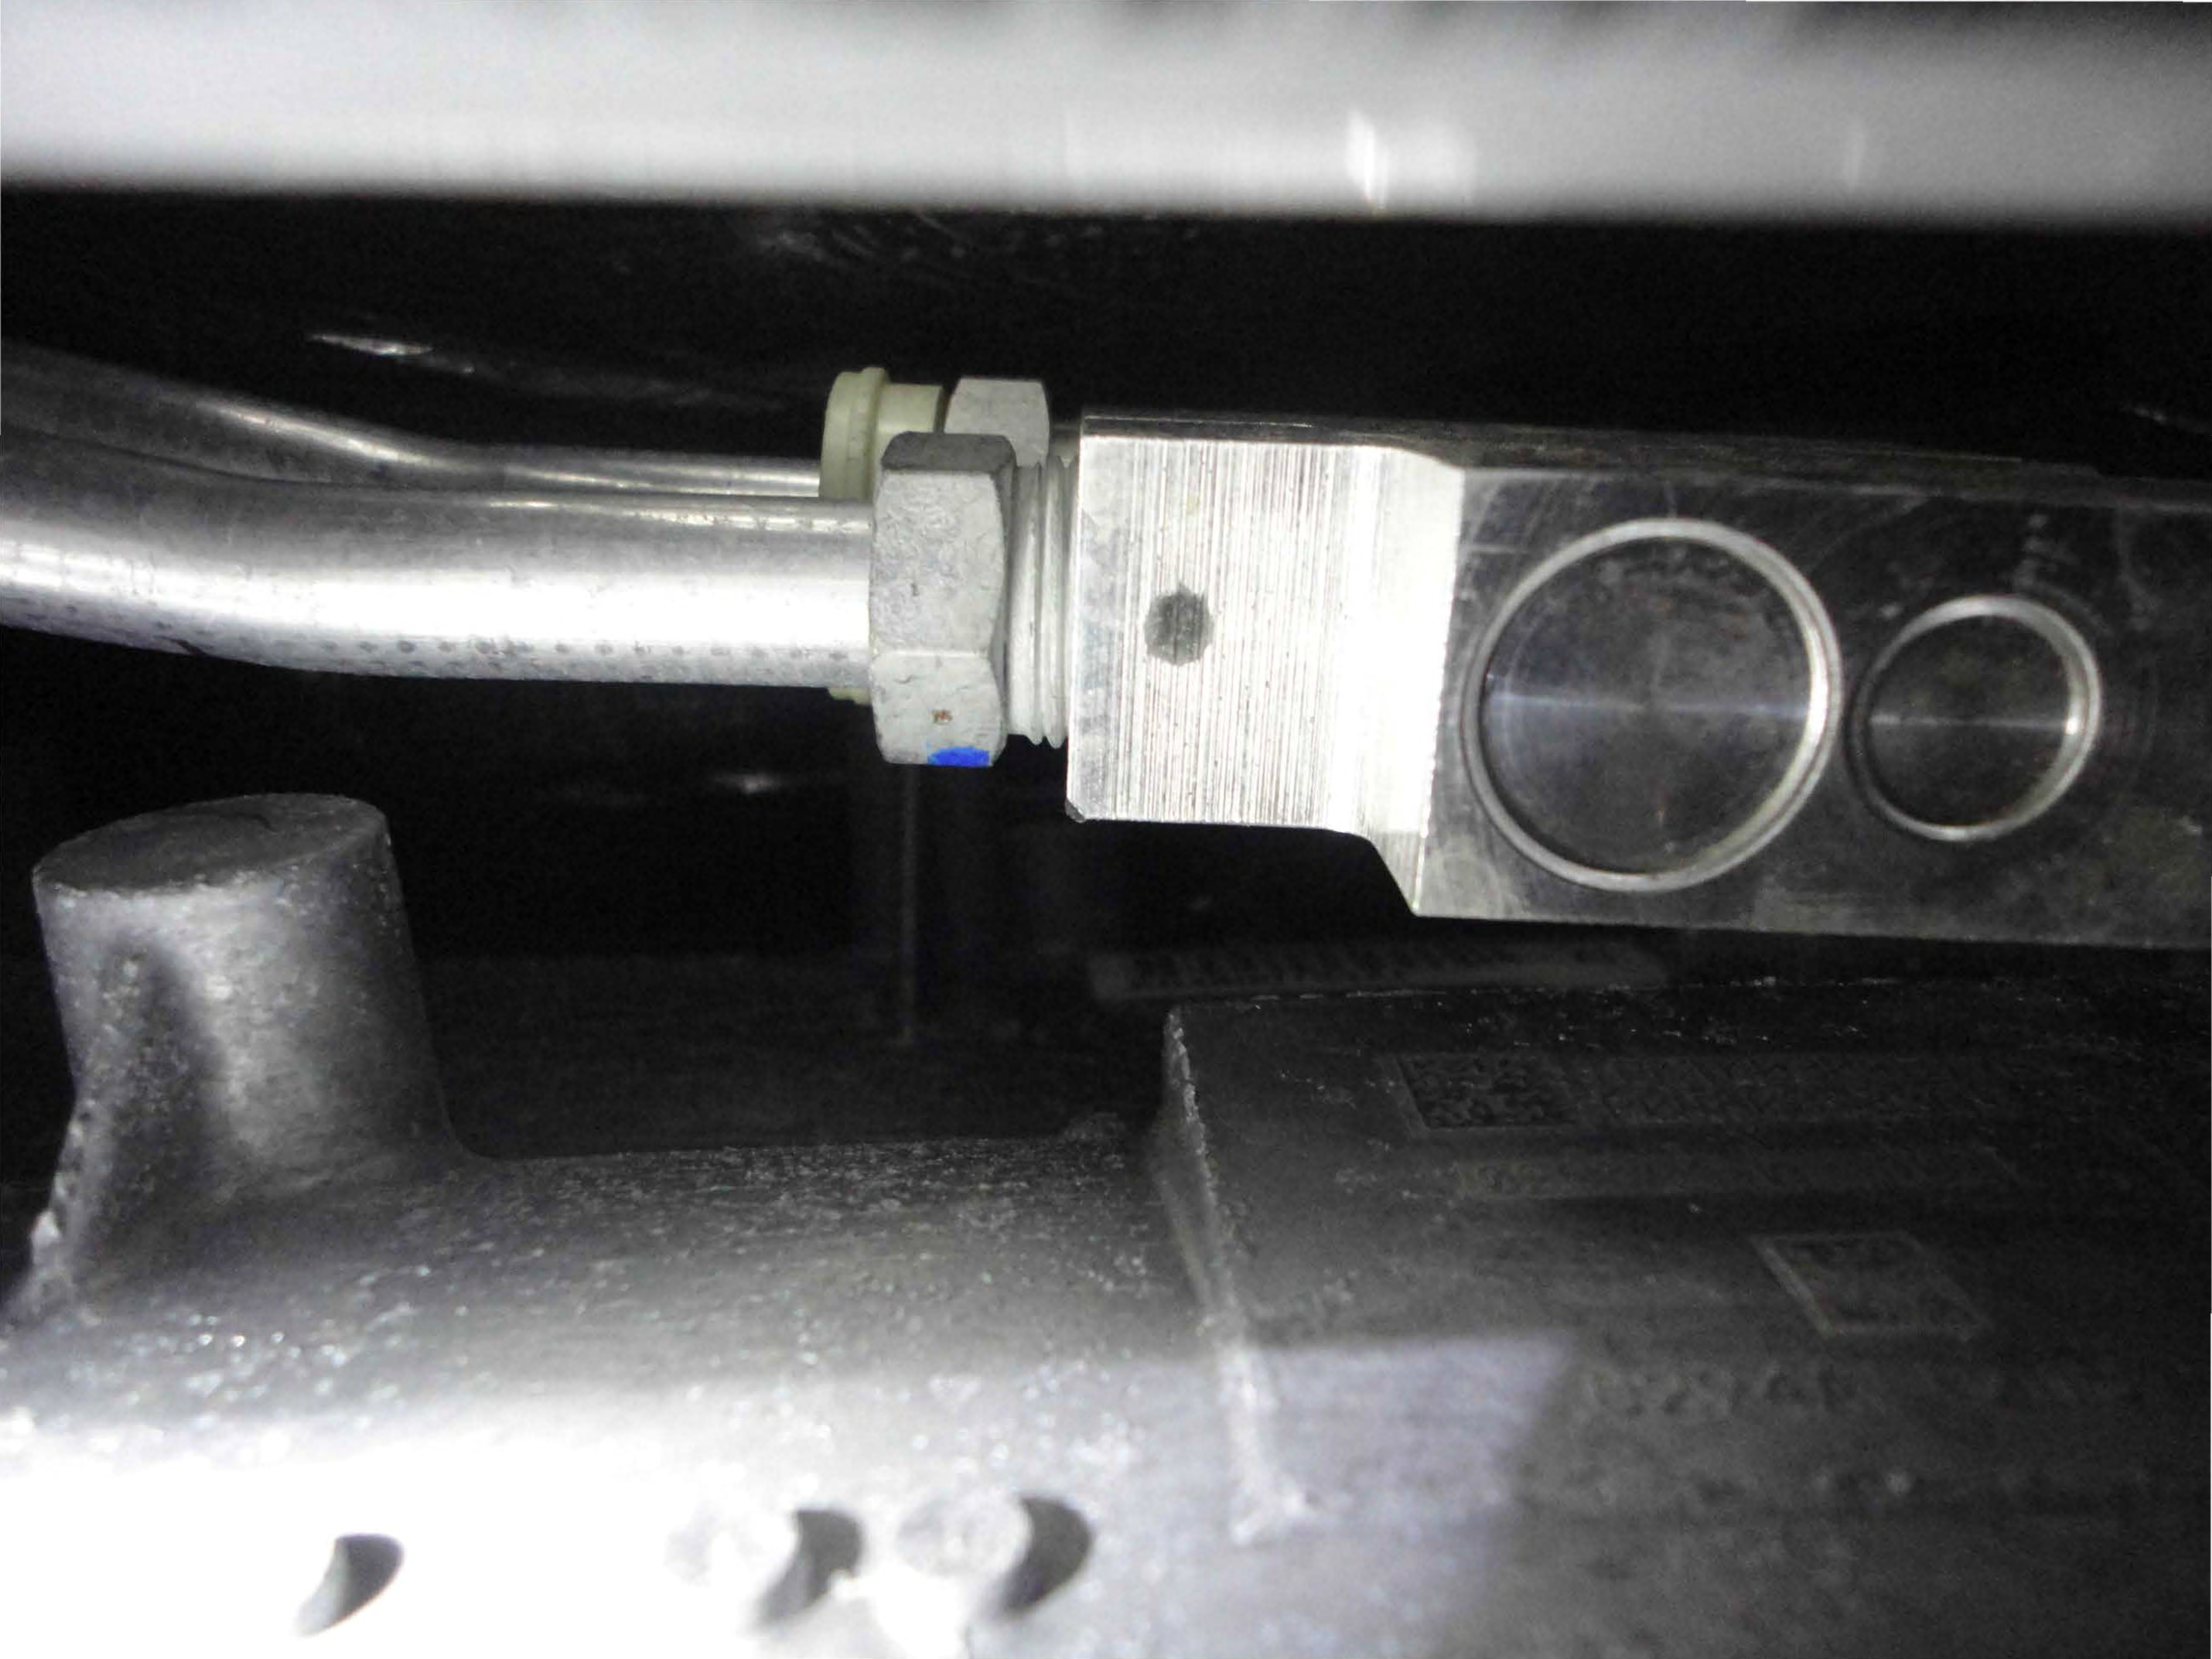

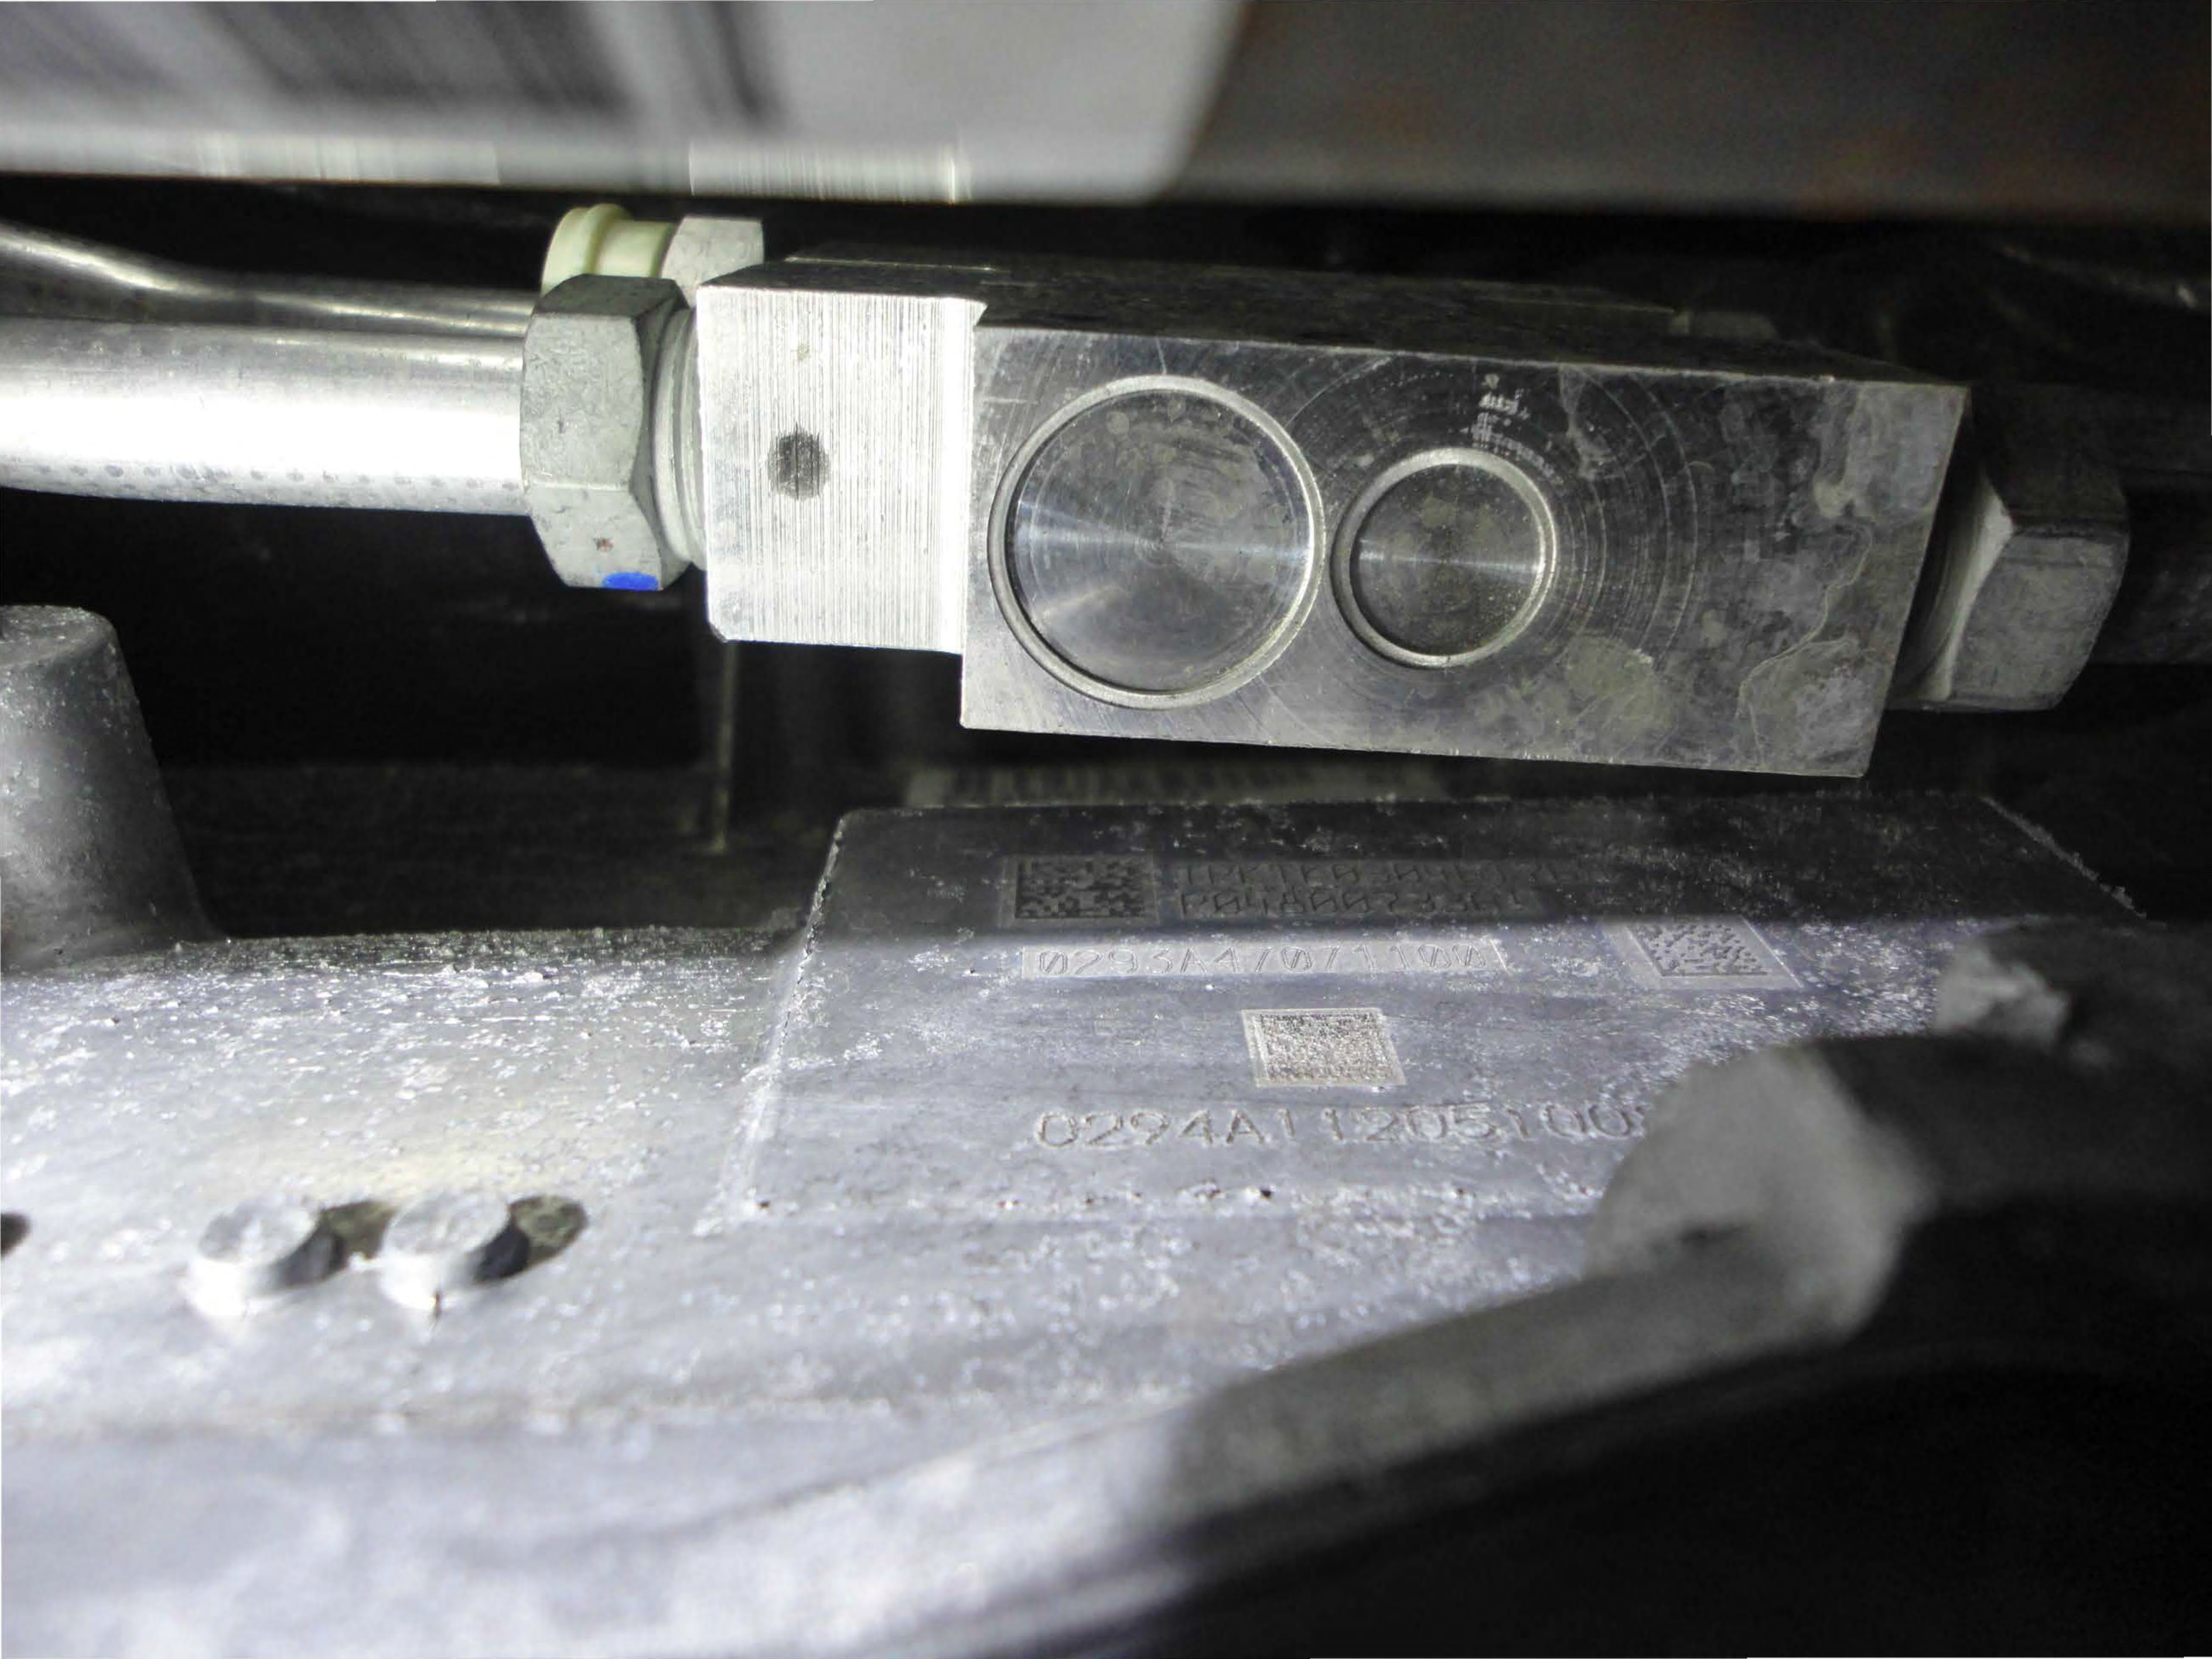

0293A47071100

0294A11205100

0294A11205100

